



Microperimeter
MP-3





THE ART OF EYE CARE



MP-3 Microperimeter

The Automatic Microperimeter with a Non-mydrriatic Fundus Camera

There have been significant advances in the assessment of retinal morphology since the incorporation of optical coherence tomography (OCT) into clinical practice. Additionally, microperimetry has advanced functional evaluation of the retina. The MP-3 measures local retinal sensitivity for functional assessment of the retina and uses the results to provide biofeedback exams for training low vision patients.

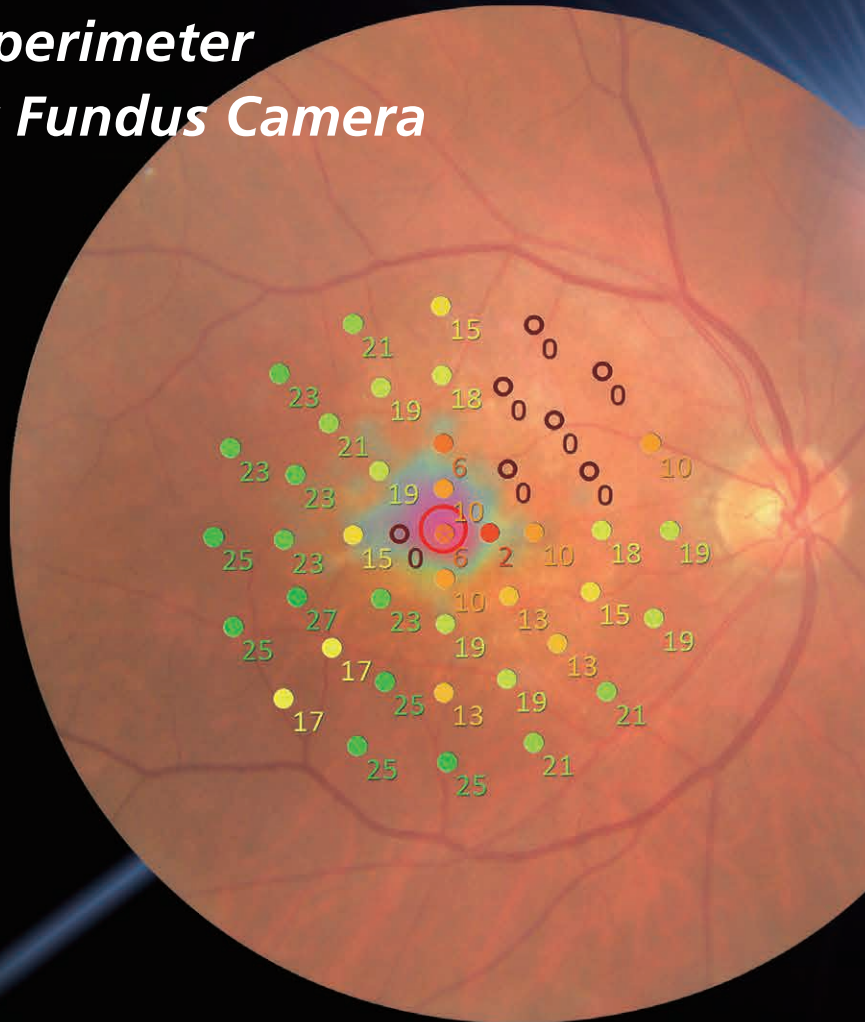

Lecture



Functional Loss in GA
By Ursula Schmidt-Erfurth, MD

https://www.nidek-intl.com/education/video_lib/special/entry-3469.html



Microperimetry: The Link between Structure and Function in AMD
By Anna Tan, MD

https://www.nidek-intl.com/education/video_lib/special/entry-3645.html



Article



Correlation of OCT Angiography and Microperimetry in Wet AMD
By Manish Nagpal, MS, DO, FRCS(Edin); Jayesh Khandelwal, MS; Rakesh Juneja, MS; and Navneet Mehrotra, MBBS, DNB (Ophthalmology), FRF

https://www.nidek-intl.com/education/case_report/retina/mp3/entry-2961.html

■ **Functionality**

Microperimetry

-Wide Measurement Range


The MP-3 has a wider range of stimulus intensity, from 0 to 34 dB, compared to the MP-1. The MP-3 measures perimetric threshold values, even for normal eyes. A maximum stimulus luminance of 10,000 asb* allows evaluation of low-sensitivity.

* In accordance with ISO12866 measurement methods

Fixation Test

-Precise Tracking System


The MP-3 can measure fixation and determine the preferred retinal locus, simply by having the patient fixate on a target. Constant tracking of the eye during microperimetry allows evaluation of fixation in patients with central visual field defects and determines whether fixation improves after treatment.

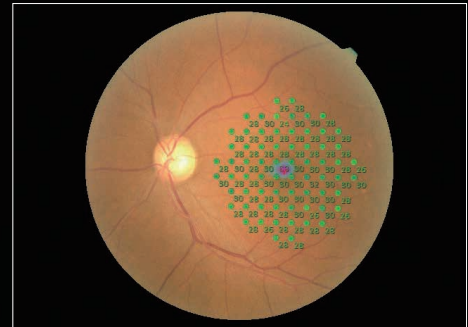

MP-3 Normal Eye Image (34 dB)



Stable Fixation

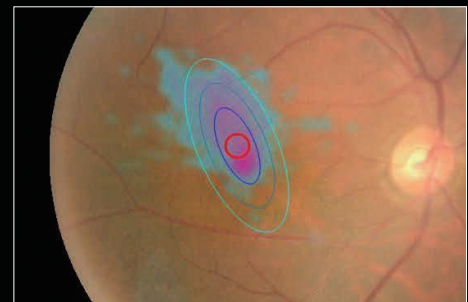

Unstable Fixation

■ **Morphology**

Retinography

-High Resolution Non-mydratiac Fundus Camera

An easy to use 12-megapixel fundus camera is incorporated into the MP-3 and acquires high resolution images of retinal pathology.




Fundus Camera Image

Precise Measurements and Follow-up

Auto Tracking and Auto Alignment

Auto tracking and auto alignment functions provide more accurate measurements increasing patient and operator comfort and efficiency. These functions allow easy follow-up and reduce variations between examiners, resulting in well-aligned follow up exams.

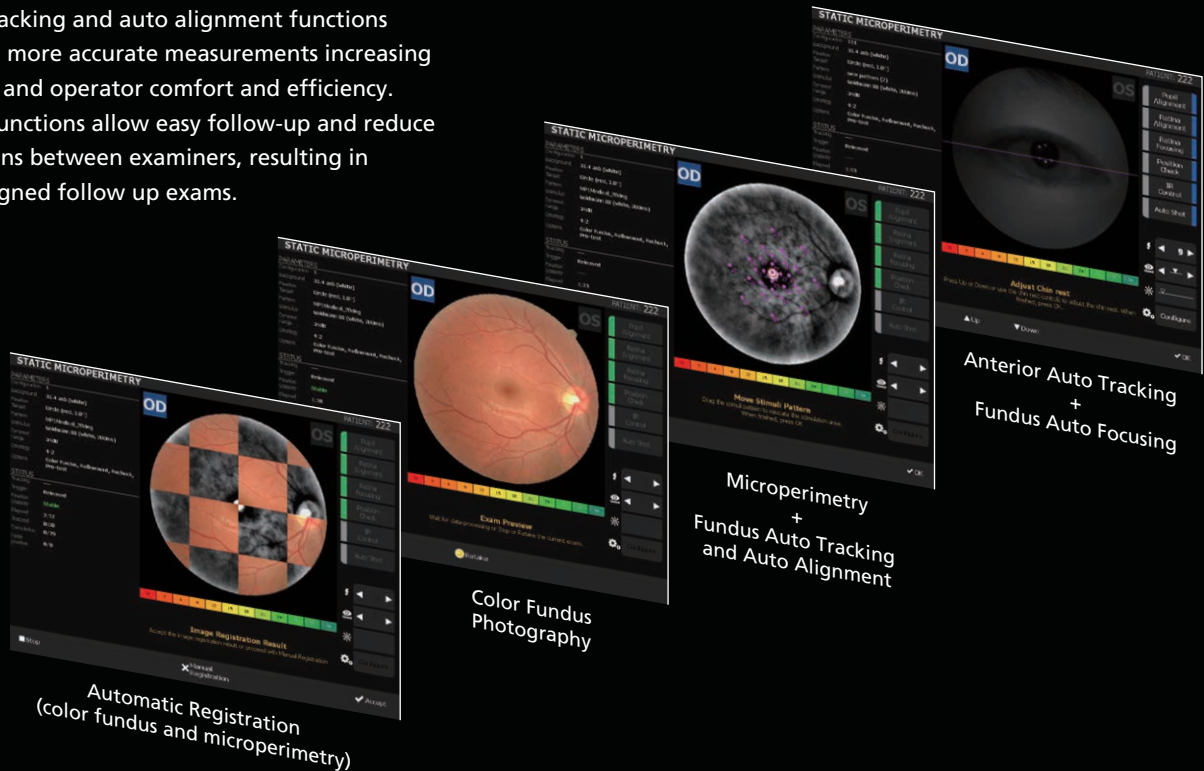

Anterior Auto Tracking + Fundus Auto Focusing

Microperimetry + Fundus Auto Tracking and Auto Alignment


Color Fundus Photography

Automatic Registration (color fundus and microperimetry)

Evaluation of Treatment

Region-specific Test Evaluation


After completion of measurements, results can be evaluated in a specific region of interest to allow easier comparison with other pathology images. By specifying the region of interest, the average results in the region are displayed.

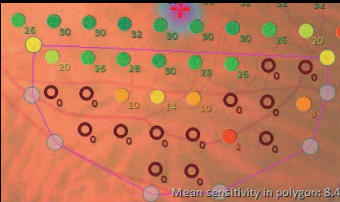

Magnified Image of Specified Fixation Point

Follow-up Test

A follow-up test can be performed on the same area using the same parameters as a previous test. This feature allows evaluation of disease progression or assessment of pre- and post-treatment outcomes. Any differences in two microperimetry images are displayed for quick, intuitive interpretation.

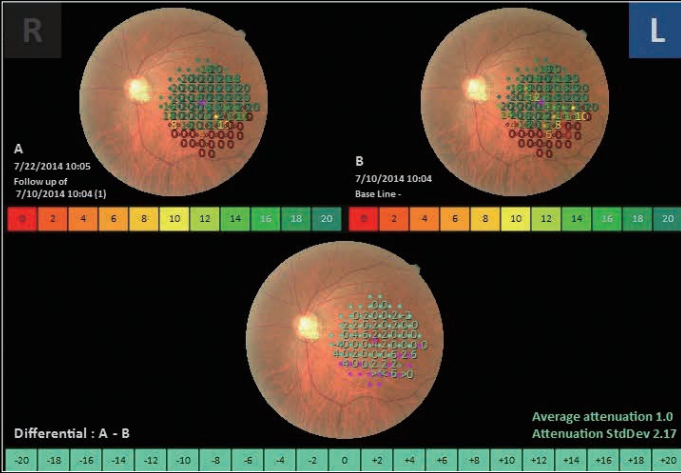

Follow-up Image

Visual Rehabilitation

Feedback Exam

The visual rehabilitation mode trains low-vision patients who have lost foveal fixation to relocate their preferred retinal locus (PRL) to a different region, called the trained retinal locus (TRL). The TRL is predetermined by a physician, and fixation rehabilitation allows the patient better functional vision (i.e. reading speed) due to increased fixation stability and visual outcomes.

Active flickering pattern stimulation and cheery music create an effective and pleasant training experience for the patient.

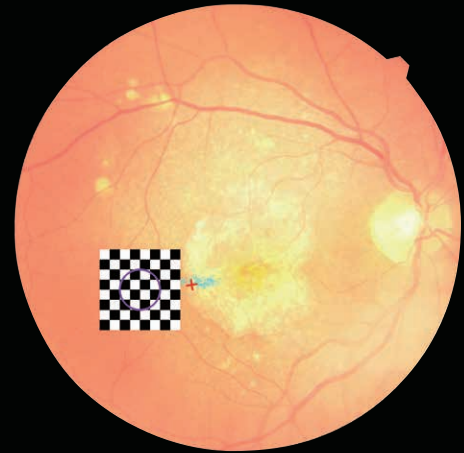


Image courtesy of the National Centre of Services and Research for the Prevention of Blindness and Rehabilitation of Visually Impaired - IAPB Italia Onlus, Rome - Italy

Related Article



Active Visual Rehabilitation: A New Paradigm in Low Vision Services

By Filippo Amore, MD, PhD

https://www.nidek-intl.com/education/case_report/retina/mp3/entry-3612.html

Functional Assessment in Scotopic Conditions (Available for the MP-3 type S)

Scotopic Microperimetry

The MP-3 type S measures retinal functions under scotopic conditions (scotopic microperimetry) in addition to the standard functions of the MP-3.


Scotopic microperimetry is used to assess the changes in rod sensitivity of degenerative retinal diseases including age-related macular degeneration and some forms of retinitis pigmentosa. This modality can be used in clinical trials of new therapeutics for retinal diseases that impair rod function.



User-friendly Functions


NAVIS-EX

NAVIS-EX is image filing software that networks the MP-3 and other NIDEK fundus imaging devices.

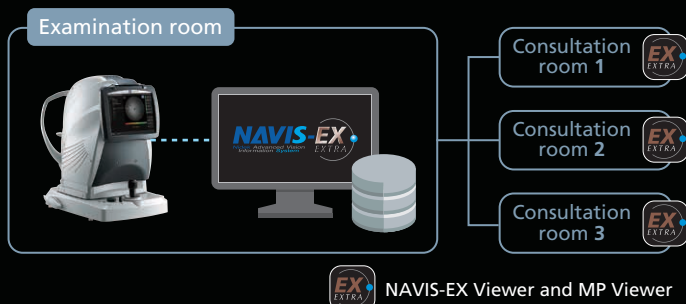

Print Setup


Various printed reports are available including user specified layouts when used with NAVIS-EX.

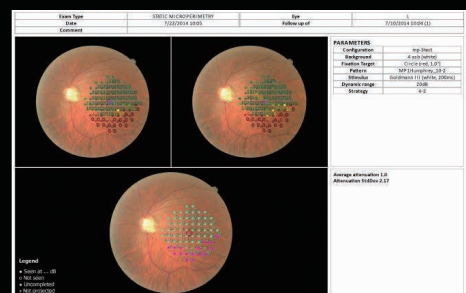

Print Image


Pre- and Post-treatment Comparison

Case of anti-VEGF treatment for age-related macular degeneration (AMD)

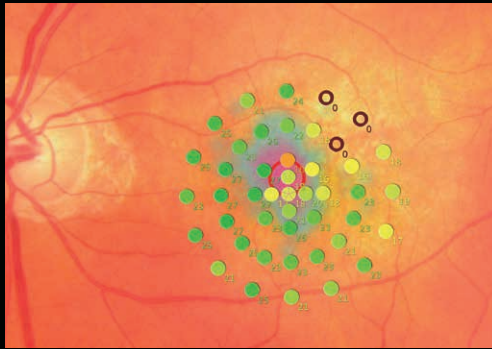

Pre-treatment


Circle at 2° Percentage of fixation points 66.1%
 Circle at 4° Percentage of fixation points 92.1%
 Mean sensitivity: 20.4

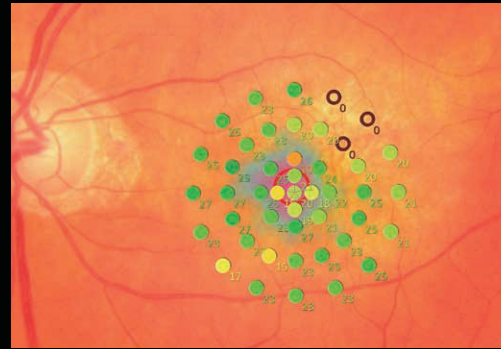


Post-treatment

Circle at 2° Percentage of fixation points 68.1%
 Circle at 4° Percentage of fixation points 95.5%
 Mean sensitivity: 20.9

Clinical Examples

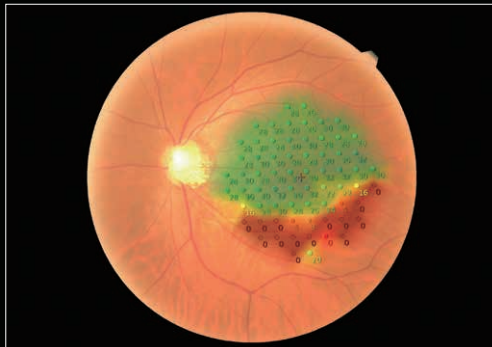


Glaucoma

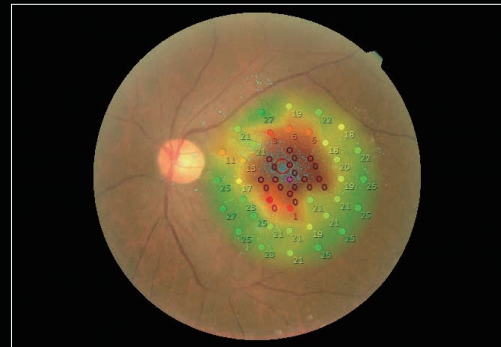


Age-related Macula Degeneration
(Geographic Atrophy)



Polypoidal Choroidal Vasculopathy

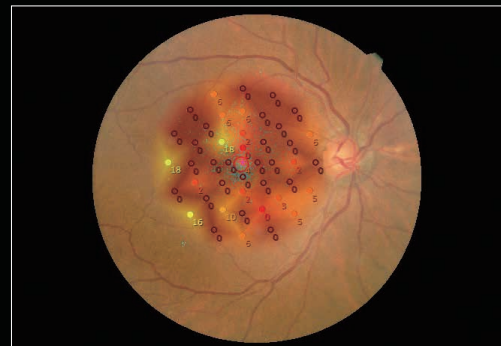

Retinal Angiomatous Proliferation

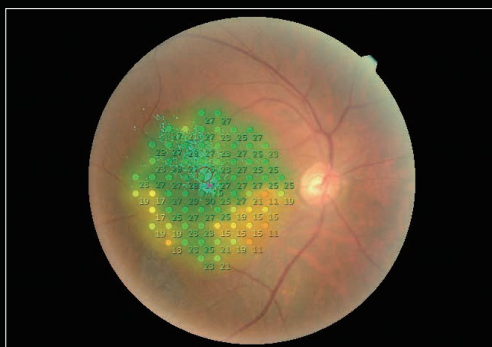

Central Serous Chorioretinopathy




Excessive Myopia

Structural and Functional Evaluation Using OCT

Evaluate retinal structure and function simultaneously using combined OCT and Microperimetry images

Various OCT modalities can be registered with Microperimetry.

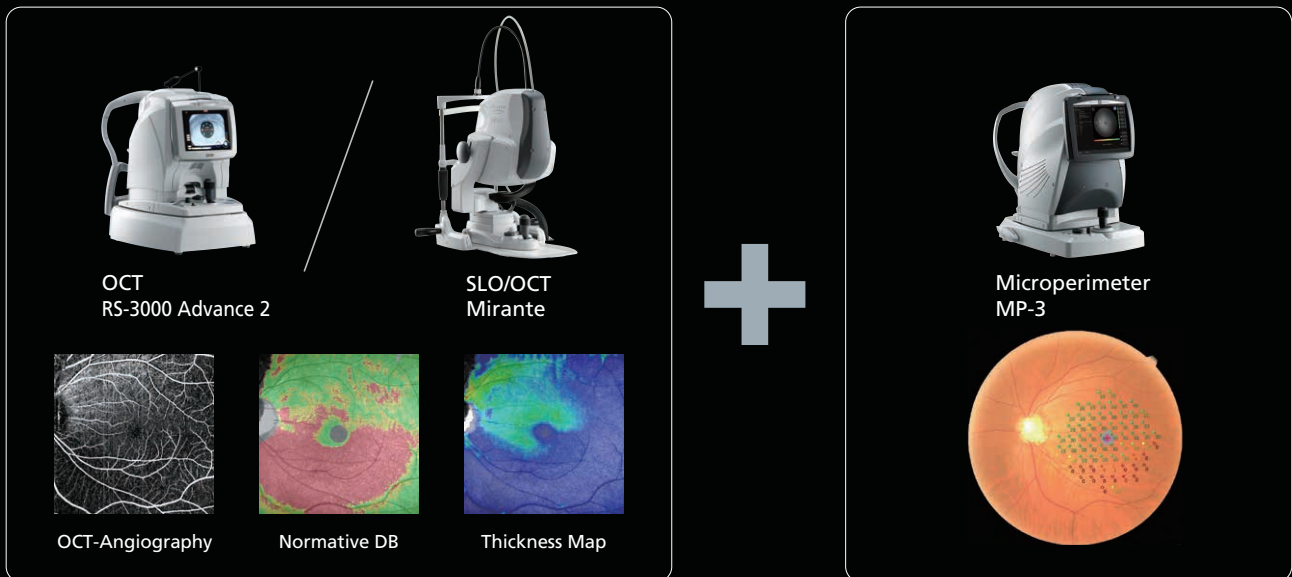

Age-related Macular Degeneration

Diabetic Macular Edema

Glaucoma

Images courtesy of Prof. S. Rizzo, MD and Dr. D. Bacherini, MD, University of Florence

MP-3 Specifications

| | |
|-----------------------------------|--|
| Microperimetry | |
| Visual field | 40° |
| Maximum stimulus luminance | 10,000 asb (in accordance with ISO12866 measurement methods) |
| Background luminance | 31.4 asb / 4 asb (in accordance with ISO12866 measurement methods) |
| Stimuli luminance threshold range | Scotopic microperimetry test*: 0.003 asb Standard [Background luminance: 31.4 asb] 10,031.4 asb (0 dB) to 35.4 asb (34 dB)(Contrast: 319.5 to 0.13) Equivalent to NIDEK MP-1 [Background luminance: 4 asb] 404 asb (0 dB) to 8 asb (20 dB) (Contrast: 101 to 1.01) 1,004 asb (0 dB) to 4.4 asb (34 dB) (Contrast: 251 to 0.1) Scotopic microperimetry test* [Background luminance: 0.003 asb] 0.303 asb (0 dB) to 0.0042 asb (24 dB) (Contrast: 101 to 0.4) |
| Stimulus size | Goldman I/II/III/IV/V compatible |
| Threshold strategy | 4-2 / 4-2-1 |
| Fixation target | Shape: single-cross, circle, four-crosses, four-lines Color: select from white/yellow/red/blue |
| Fundus Camera | |
| Type | Non-mydratic fundus camera, color |
| Angle of view | 45° ±5% (The refraction of the eye is 0 D) |
| Minimum pupil diameter | ø4 mm |
| Camera | Built-in 12-megapixel CCD camera |
| Auto tracking | X-Y-Z directions |
| Auto shot | Available |
| Working distance | 45.7 mm |
| Display | 10.4-inch color LCD touch screen |
| Diopter correction range | -25 to +15 D |
| Fundus auto focus range | -12 to +15 D |
| Power supply | 100 to 240 V AC 50/60 Hz |
| Power consumption | 160 VA |
| Dimensions/mass | 334 (W) x 562 (D) x 560 (H) mm / 36 kg 13.1 (W) x 22.1 (D) x 22.0 (H) " / 79 lbs. |
| Optional accessories | Motorized optical table |

* Available for the MP-3 type S



MP-3



MP-3 type S



More clinical information available online at the NIDEK Education page

For more clinical information, please visit the Education page on the NIDEK website. This site allows access to case reports, journal articles, and video presentations.



<https://www.nidek-intl.com/education/>

Product/model name: Microperimeter MP-3

Brochure and listed features of the device are intended for non-US practitioners.

Specifications may vary depending on circumstances in each country.

Specifications and design are subject to change without notice.

 Eye & Health Care
NIDEK CO., LTD.

HEAD OFFICE
(International Div.)
34-14 Maehama,
Hiroishi-cho, Gamagori,
Aichi 443-0038, JAPAN
TEL: +81-533-67-8895
URL: www.nidek.com
[Manufacturer]

TOKYO OFFICE
(International Div.)
3F Sumitomo Fudosan Hongo
Bldg., 3-22-5 Hongo, Bunkyo-ku,
Tokyo 113-0033, JAPAN
TEL: +81-3-5844-2641
URL: www.nidek.com

NIDEK INC.
2040 Corporate Court,
San Jose, CA 95131, U.S.A.
TEL: +1-408-468-6400
+1-800-223-9044
(US Only)
URL: usa.nidek.com

NIDEK S.A.
Ecoparc,
9 rue Benjamin Franklin,
94370 Sucy En Brie,
FRANCE
TEL: +33-1-49 80 97 97
URL: www.nidek.fr

NIDEK TECHNOLOGIES S.R.L.
Via dell'Artigianato,
6/A, 35020 Albignasego (Padova),
ITALY
TEL: +39 049 8629200/8626399
URL: www.nidektechnologies.it

NIDEK (SHANGHAI) CO., LTD.
Rm3205, Shanghai Multi
Media Park, No.1027 Chang
Ning Rd, Chang Ning District,
Shanghai, CHINA 200050
TEL: +86 021-5212-7942
URL: www.nidek-china.cn

NIDEK SINGAPORE PTE. LTD.
51 Changi Business Park
Central 2, #06-14,
The Signature 486066,
SINGAPORE
TEL: +65 6588 0389
URL: www.nidek.sg